First Medical Source

Delivering Safe & Effective Infusion Systems.

Better Care for Better Life. InfuLife®

USA

InfuLife® Infusion System Patient Guide

InfuLife is a portable, single-use, sterile elastomeric pump that delivers your medication. The stretched balloon gently pushes the medication through the tubing into your body. InfuLife is not made with natural rubber latex or DEHP. It is made in an ISO 13485-certified facility, in an ISO Class 8 (Class 100,000) cleanroom. The InfuLife System consists of the pump and its carry pouch.



Important points

- The medication should infuse over _ minutes/hours. Your provider will also tell you how long the infusion should last.
- There are no alarms to tell you when the medication is done infusing. Check the back of the balloon to see how much medication has been infused. The markings give only a general idea of how much medication is left.



- As the medication is infused, the balloon is getting smaller. When the balloon is flat, with the end of the hard core at the center, you've received all your medication.



- Put InfuLife in the carry pouch provided. This pouch allows you to carry the pump around your belt when you are mobile and hang it at your bedside at night.
- Solutions colder than room temperature take longer to infuse.



Solutions warmer than room temperature will infuse faster.

- Flow rates are calculated with the pump at the same height as your catheter site. For best accuracy, keep the pump at about the same height as your catheter site.
- **Tape down and keep the**

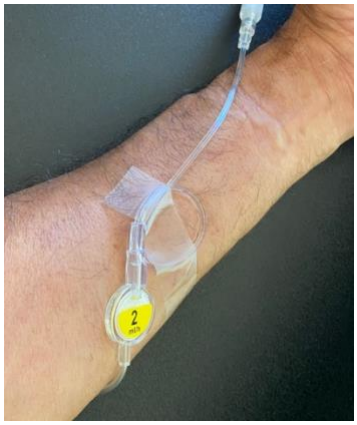

section of the tubing from the filter to the patient connector in contact with the body (see picture).

- Placing the pump under a blanket or above your catheter site will make the medication flow faster.
- Do not heat InfuLife**.** Using a heat source such as microwave oven, direct sunlight or hot water to heat InfuLife may affect how the device works and how fast the medication is infused.
- When the InfuLife is at room temperature inspect for leaks on the entire device.
- Avoid sharp rigid objects from contacting the flexible membranes of the pump body.
- Do not seal off the vent hole on the inline filter.
- Do not bathe or swim with InfuLife. You may shower if the pump and your catheter site are protected from water.
- If your pump contains fluorouracil (5-FU), do not refrigerate it or let it get cold.
- When the infusion is finished, close the clamp, disconnect the pump as your provider showed you, and dispose of it as instructed.

Troubleshooting

If the pump doesn't seem to be working, make sure:

- All clamps on your catheter are open.
- There are no kinks in the pump tubing.



- The white clamp on the tubing is open.
- The pump is at room temperature, and there is no leakage.
- At slow rates (below 2 mL per hour), it can take a while for a drop to form at the end of the tubing. This is normal.

- Follow your provider's instructions. Call your provider if the problem persists.
- Call your provider right away if the pump or tubing leaks or is wet; if you have pain, swelling, redness or leakage at your catheter site; if you feel unwell; or if the balloon is not getting smaller as expected.

This information is not a substitute for medical advice or treatment. Consult your physician or healthcare provider about this information and any health-related questions you have. FMS assumes no liability whatsoever for the information provided or for any diagnosis or treatment made based on this information.

For additional information, please visit https://www.infulife.com or contact support@firstmedicalsource.com.

InfuLife® Patient Guide, PMP-1102 Rev B · © 2026 First Medical Source, LLC